


COMPONENTS



PRODUCT CODES

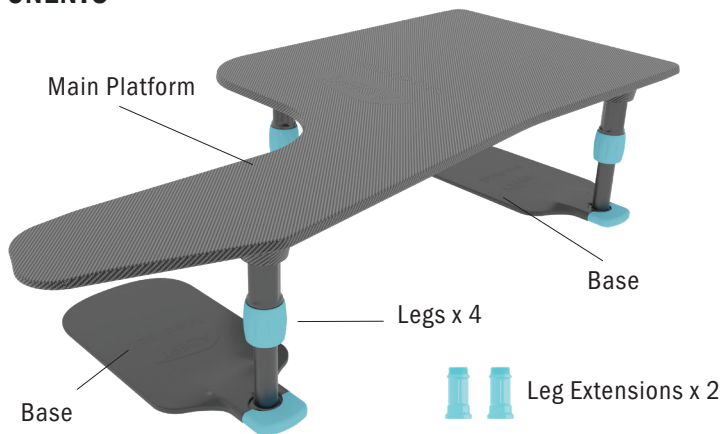


AM0440

Antegrade IR Platform


UNBOXING

1

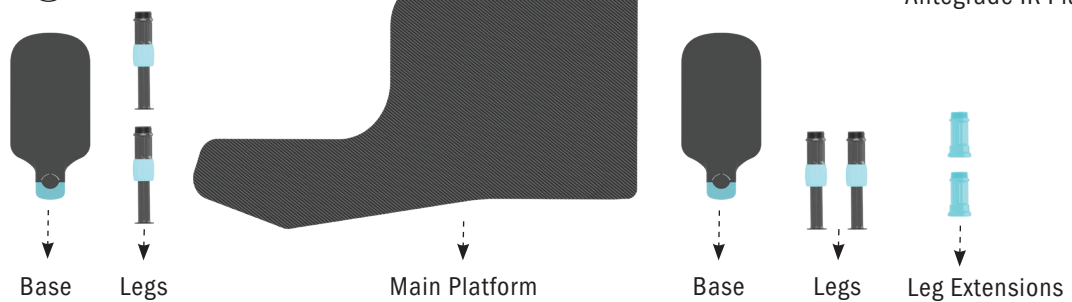

AM0440

Antegrade IR Platform

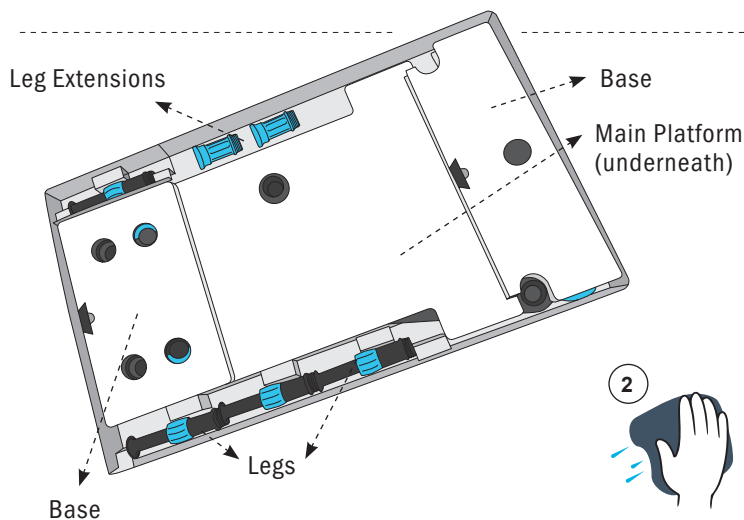


CLEANING



Disinfect and wipe clean before/after each use.

DO NOT USE any other sterilisation methods.

ASSEMBLY

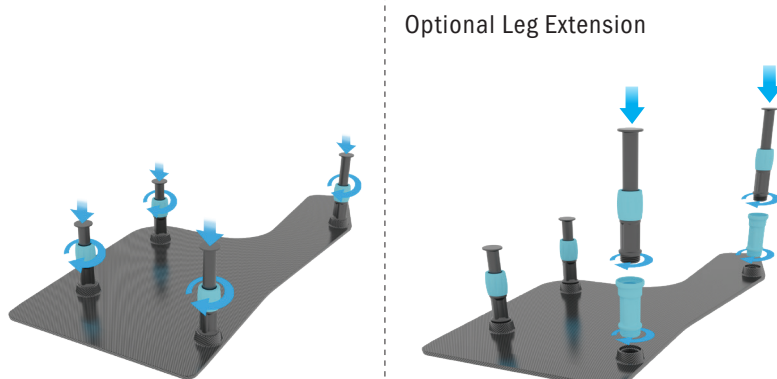

For an online training visit:
AdeptMedicalTraining.com



For service and repairs visit
AdeptMedical.com/repairs



For Approved Disinfectants PDF visit:
AdeptMedical.com/antegrade-ir-platform

MANUFACTURER

Adept Medical Ltd
2-6 McDonald St, Morningside
Auckland 1025, New Zealand
www.adeptmedical.co.nz


EC REPRESENTATIVE

Emargo Europe
Prinsessegracht 20
2514 AP The Hague
The Netherlands

EC REP




SETUP

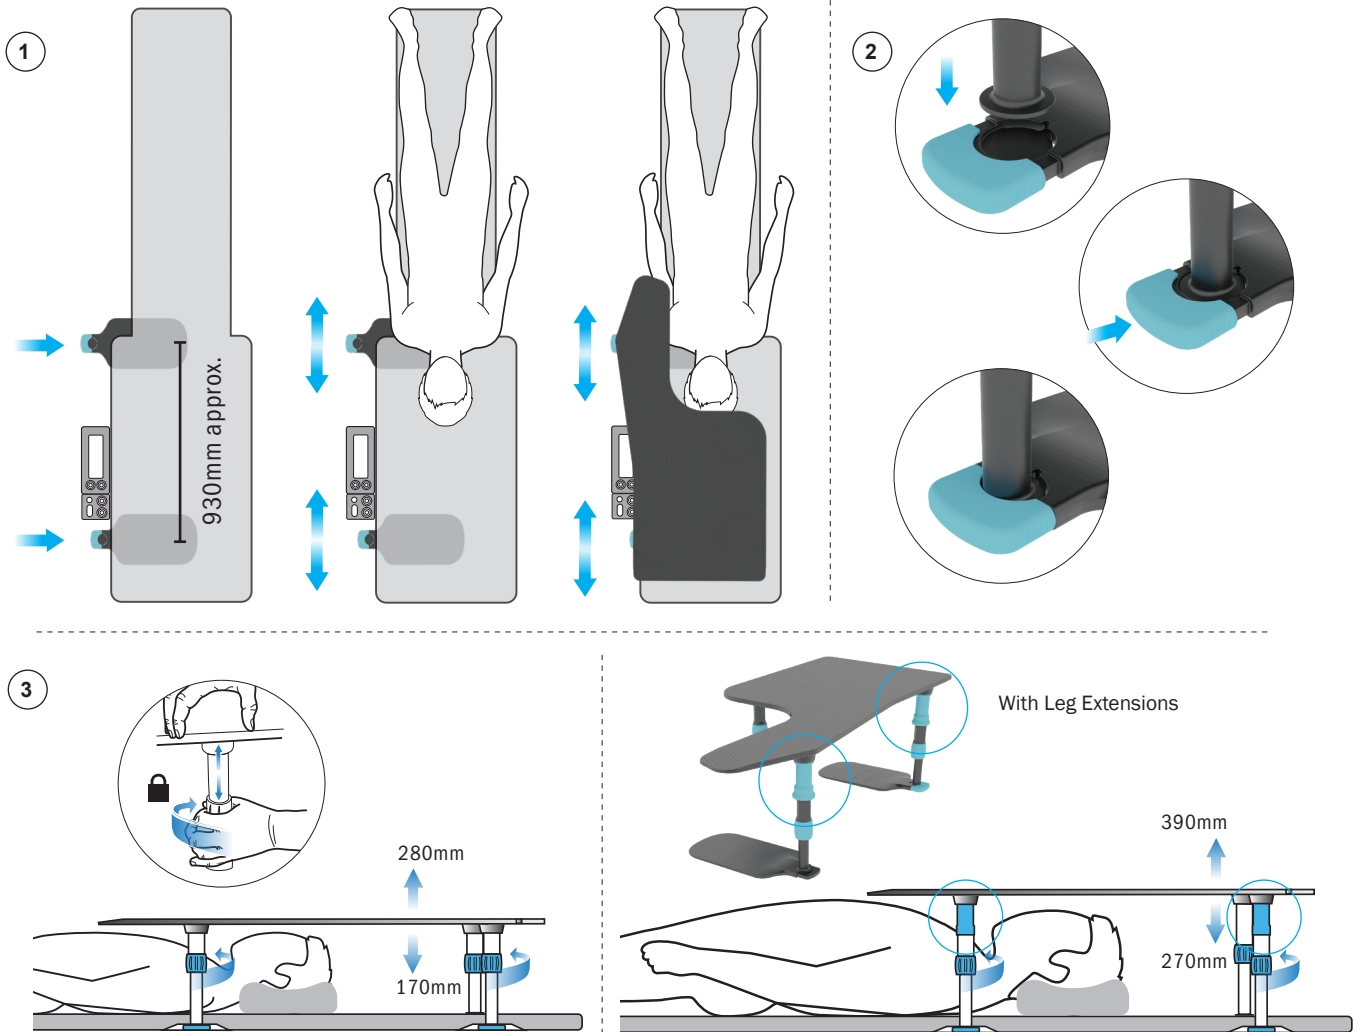

DRAPE SUPPORT (AM1000)

Optional

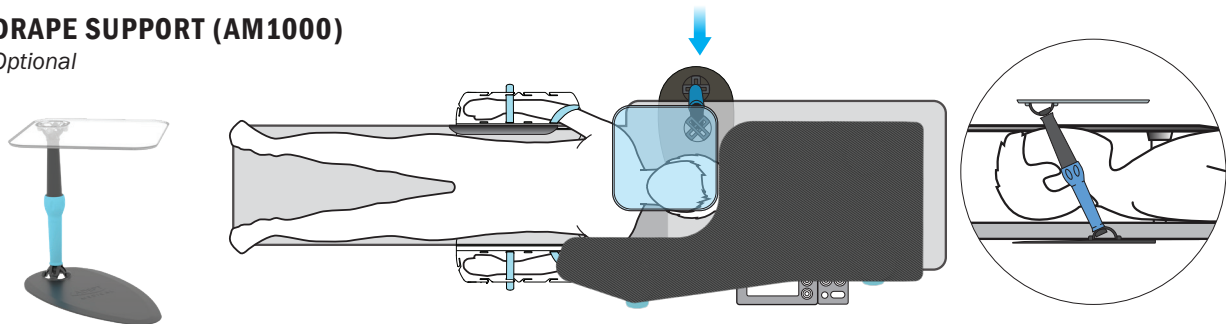

*Drape Support is not included with the Antegrade IR Platform.

